OMRON

3125186-3A

Upper Arm **Blood Pressure Monitor**

Model HEM-7600T Instruction Manual

Introduction

Thank you for purchasing the OMRON Upper Arm Blood Pressure Monitor. Your new upper arm blood pressure monitor uses the oscillometric method of blood pressure measurement. This means the monitor detects your blood movement through your brachial artery and converts the movements into a digital reading. An oscillometric monitor does not need a stethoscope so the monitor is simple to use

Intended Use

This device is a digital monitor intended for use in measuring blood pressure and pulse rate in adult patient population. The device detects the appearance of irregular heartbeats during measurement and gives a warning signal with readings. It is mainly designed for general household use.

Important Safety Information

Please read the Important Safety Information in this instruction manual before using the unit

Please follow this instruction manual thoroughly for your safety. Please keep for future reference. For specific information about your own blood pressure, CONSULT YOUR DOCTOR.

Indicates a potentially hazardous situation which, if not avoided, could result in death or serious injury. A Warning

- DO NOT adjust medication based on measurement results from this blood pressure monitor. Take medication as prescribed by your doctor. Only a doctor is qualified to diagnose and treat high blood pressure
- · DO NOT use this monitor on an injured arm or an arm under medical treatment
- · DO NOT wear the arm cuff on your arm while on an intravenous drip or blood transfusion
- · DO NOT apply or inflate the arm cuff around any body parts other than your upper arm
- DO NOT use this monitor in areas containing high frequency (HF) surgical equipment, magnetic resonance imaging (MRI) equipment, computerized tomography (CT) scanners or in oxygen rich environments. · DO NOT use this monitor on infants, toddlers, children or persons who cannot
- express themselves. · Consult your doctor before using this monitor if you have common arrhythmias
- such as atrial or ventricular premature beats or atrial fibrillation; arterial sclerosis; poor perfusion; diabetes; pregnancy; pre-eclampsia; or renal disease
- · Always consult your doctor. Self-diagnosis of measurement results and self-treatment are dangerous.
- · Contains small parts that may cause a choking hazard if swallowed by children, toddlers or infants.
- · Keep the BATTERY out of the reach of children, toddlers and infants. This product emits radio frequencies (RF) in the 2.4 GHz band. DO NOT use this product in locations where RF is restricted, such as on an aircraft or in hospitals

Indicates a potentially hazardous situation which, if not avoided, may result in minor or moderate injury to the user or patient or damage to the equipment or other **≜**Caution property.

· Stop using this monitor and consult your doctor if you experience skin irritation or discomfort

- · Consult your doctor before using this monitor on an arm with an arterio-venous (A-V) shunt
- · Note that PATIENT motion, trembling, shivering may affect the measurement reading · Consult your doctor before using this monitor if you have had a mastectomy.
- · Consult your doctor before using the monitor if you have severe blood flow problems or blood disorders as cuff inflation can cause bruising.
- Do not take measurements more often than necessary because bruising, due to blood flow interference, may occur.
- Remove the arm cuff if it does not start deflating during the measurement. · Do not use this monitor for any purpose other than measuring blood pressure.
- · Do not use a mobile phone or other electrical devices that emit electromagnetic fields near this monitor except when transferring your readings to your smart device. This may result in incorrect operation of this monitor. · Do not disassemble or attempt to repair the monitor or components. This may
- cause an inaccurate reading. · Do not use in a location where there is moisture or a risk of water splashing the
- monitor. This may damage the monitor. · Do not use this monitor in a moving vehicle such as in a car or on an airplane.
- · Do not drop, or subject this monitor to strong shocks or vibrations
- Do not use this monitor in places with high or low humidity or high or low temperatures. See the "6. Specifications" section of the manual.
- · Please check, by observation of the arm being used, that the monitor is not
- rment of patient blood circu · Do not use this monitor in high-use environments such as medical clinics or
- doctor offices · Avoid bathing, drinking alcohol or caffeine, smoking, exercising and eating for
- 30 minutes before taking a measurement. • Rest for at least 5 minutes before taking the measurement.
- · Remove tight-fitting or thick clothing from your arm while taking a
- measurement
- · Remain still and do not talk while taking a measurement. Read and follow the "Important information regarding Electro Magnetic
- Compatibility (EMC)" in the EMC information provided with this device.
- Read and follow the "Correct Disposal of This Product" in "6. Specifications" when disposing of the device and any used accessories or optional parts.

Data Transmission

- · Do not replace the battery while your reading is being transferred to your smart device. This may result in the incorrect operation of your monitor and failure to transfer your blood pressure data.
- Do not place integrated circuit cards, magnets, metal objects, or other devices that emit electromagnetic fields near this monitor while your reading is being transferred to your smart device. This may result in the incorrect operation of your monitor and failure to transfer your blood pressure data.

Battery Handling and Usage

- Do not insert the batteries with their polarities incorrectly aligned.
- · Use only 4 "AAA" alkaline batteries with this monitor. Do not use other types of batteries. Do not use new and used batteries together. · Remove the batteries if the monitor will not be used for a long period of time.
- If battery fluid should get in your eyes, immediately rinse with plenty of clean water. Consult a doctor immediately.


- · If battery fluid should get on your skin, wash your skin immediately with plenty of clean, lukewarm water. If irritation, injury or pain persists, consult a doctor. Do not use batteries after their expiration date.
- Periodically check your batteries to ensure they are in good working condition. · Only use batteries specified for this monitor. Use of unsupported batteries may damage and/or may be hazardous to the monitor.


1. Know Your Device

Contents:

Monitor, battery set, instruction manual, setup instructions

Monitor:

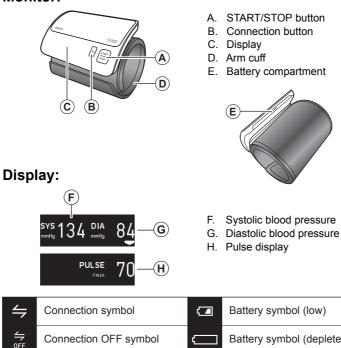

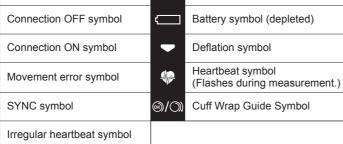

Irregular Heartbeat

Blood pressure

Blood pressure

1.1 Display symbols

<u>"</u>A

 \leq

 \bigcirc

Irregular Heartbeat Symbol (2)

When the monitor detects an irregular rhythm two or more times during the measurement, the

irregular heartbeat symbol will appear on the display with the measurement values. An irregular heartbeat rhythm is defined as a

rhythm that is 25% less or 25% more than the average rhythm detected while the monitor is measuring the systolic and diastolic blood

pressure

If the irregular heartbeat symbol displays with your measurement results, we recommend you consult your doctor. Follow the directions of your doctor.

Movement Error Symbol ()

The movement error symbol is displayed if you move your body during the measurement. Please remove the arm cuff, and wait 2 - 3 minutes. Take another measurement and remain still during measurement.

Cuff Wrap Guide Symbol (/)

If the cuff was wrapped too loosely, it may cause unreliable results. If the wrapping of cuff is too loose, the cuff wrap guide symbol "O" appears. determining if the cuff is wrapped snugly enough.

- SYNC Symbol ()
- · When the SYNC symbol appears on the display, make sure that your monitor has been pairing with the smart device or transfer the data.

· When the SYNC symbol appears on the display, transfer the data before the measurements are deleted. If the memory is full, the monitor will be delete the oldest value. Maximum internal memory is for 100 measurements

2013 ESH/ESC Guidelines for the management of arterial hypertension Definitions of hypertension by office and home blood pressure levels


,, ,			
	Office	Home	
Systolic Blood Pressure	≥140 mmHg	≥135 mmHg	
Diastolic Blood Pressure	≥90 mmHg	≥85 mmHg	
These are from statistical values for blood pressure.			

1.2 Before Taking a Measurement

- To help ensure an accurate reading, follow these directions: 1. Avoid bathing, drinking alcohol or caffeine, smoking, exercising and
- eating for 30 minutes before taking a measurement. 2. Rest for at least 5 minutes before taking the measurement.
- 3. Stress raises blood pressure. Avoid taking measurements during stressful times.
- 4. Measurements should be taken in a quiet place.
- 5. Remove tight-fitting clothing from your arm.
- 6. Keep a record of your blood pressure and pulse readings for your doctor. A single measurement does not provide an accurate indication of your true blood pressure. You need to take and record several readings over a period of time. Try to measure your blood pressure at the same time each day for consistency.

2. Preparation

- 2.1 Battery Installation
- **1.** Remove the battery cover. Gently slip into the gap of the hook and pull downward.

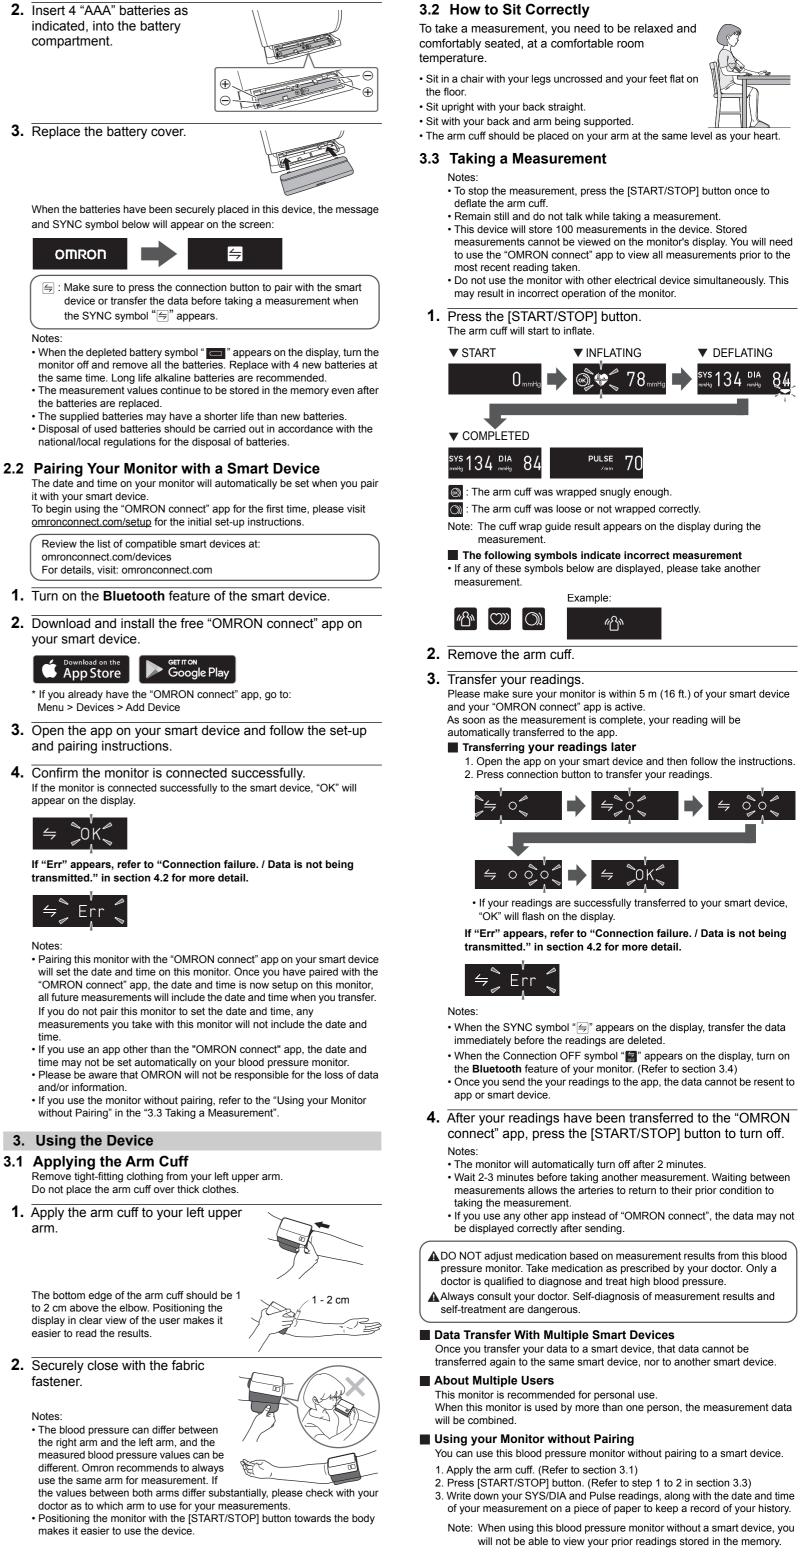

2.2 Pairing Your Monitor with a Smart Device







- 3.4 Turning "OFF" Bluetooth Turn off the Bluetooth in your monitor in the following areas where use of wireless equipment is prohibited. • On aircraft • In hospitals • While abroad Your blood pressure monitor comes with the **Bluetooth** already turned on.
- **1.** Turn your monitor power off if it is turned on.
- **2.** Press and hold the connection button for more than 10 seconds.
- **3.** Release the connection button when " $\square \rightarrow \square$ " appears on the display.



4. Press the [START/STOP] button to turn the monitor off. Note: The monitor will automatically turn off after 2 minutes.

How to turn "ON" Bluetooth

Operate the following step when the power has been off. Press and hold the connection button for more than 2 seconds and then release the connection button when " $\Rightarrow \ddagger$ " appears on the display.

- 3.5 Restoring Your Monitor to the Default Settings To delete all the information stored in your monitor, follow the instructions below. Make sure that your monitor is turned off. It is off when the screen is not showing numbers or symbols.
- **1.** While holding the connection button down, the Connection symbol "
 and "
 P" appear on the display, and then press the [START/STOP] button for more than 5 seconds.



2. When the "Clr" symbol appears on the display, release the connection button and [START/STOP] button. The "Clr" will appear on the display when your monitor settings have reverted back to their original.



- 3. Press the [START/STOP] button to turn the monitor off.
 - The monitor will automatically turn off after 2 minutes.
 - Reverting to initial settings of this monitor will not delete the information in the app
 - When using this monitor again, please delete the registration of the monitor in the app first, and then pair your monitor.

4. Error Messages and Troubleshooting

4.1 Frror Messages

+ .	_'''	U	INIC	330	ayes	•

Error Display Cause		Solution	
∽»	Irregular heartbeat is detected.	Remove the arm cuff. Wait 2 - 3 minutes and then take another measurement. Repeat the steps in section 3.1. If this error continues to appear, contact your doctor.	
"合"	Movement during measurement.	Carefully read and repeat the steps in section 3.3.	
O1	Arm cuff is applied too loosely.	Apply the arm cuff tighter. Refer to section 3.1.	
	The batteries are low.	Recommend replacement of all 4 batteries with new ones. Refer to section 2.1.	
	The batteries are depleted or battery	Immediately replace 4 batteries with new ones. Refer to section 2.1.	
	polarities are not properly aligned.	Confirm the batteries are properly inserted with polarities correctly aligned. Refer to section 2.1.	
⇔ Err	Connection failure. Data is not being transmitted.	Refer to "Connection failure. Data is not being transmitted." in section 4.2.	
E 1	Arm cuff is applied too loosely.	Apply the arm cuff tighter. Refer to section 3.1.	
E 3	The arm cuff was inflated exceeding the maximum allowable pressure, and then deflated automatically. Movement during measurement.	Do not touch the arm cuff while taking a measurement. Refer to section 3.3.	
E 4		Repeat measurement. Remain still and do not talk during measurement. Refer to section 3.3.	
E 5	Clothing is interfering with the arm cuff.	Remove any clothing interfering with the arm cuff. Refer to section 3.1.	
Er XX If the number is shown except 1 to 5.	Device error.	Contact your local OMRON representative.	

4.2 Troubleshooting

Problem	Cause and Solution
No power. No display appears on the monitor.	Replace all batteries with new ones. Check the battery installation for proper placement of the battery polarities. Refer to section 2.1.
Measurement values appear too high or too low.	Blood pressure varies constantly. Many factors including stress, time of day, and how you apply the arm cuff, may affect your blood pressure. Review the section, 3.2 and 3.3.
	The blood pressure monitor might not be properly placed within the smart device's transmission range and is too far from the smart device. If there are no causes of data transmission interference found near the blood pressure monitor, move the blood pressure monitor within 5 m (16 ft.) of the smart device and try again.
	The Bluetooth feature of the smart device is turned off. Turn on the Bluetooth feature of the smart device and your monitor, and try sending the data again.
Connection failure. /	The Bluetooth feature of the blood pressure monitor is turned off. Refer to "To turn "ON" the Bluetooth " in "3.4 Turning "OFF" the Bluetooth ".
ata is not being transmitted.	The blood pressure monitor did not pair successfully to the smart device. Try to pair the devices again. Refer to "Pair Your Monitor with a Smart Device" in section 2.2. For more detail, go to "Help" in the "OMRON connect" app.
	The application on the smart device is not ready. Check the application then try sending the data again. Refer to "Pair Your Monitor with a Smart Device" in section 2.2. If the "Err" symbol still displays after checking the application, contact your local OMRON representative. Confirm your smart device compatibility with this monitor at omronconnect.com

5. Maintenance and Storage

5.1 Maintenance

- To protect your device from damage, please follow the directions below: · Store the device and the components in a clean, safe location.
 - Do not use any abrasive or volatile cleaners.
 - . Do not wash the device and any components or immerse them in water. Do not use gasoline, thinners or similar solvents to clean the device.



· Use a soft dry cloth, or a soft cloth moistened with neutral soap to clean on the monitor and the arm cuff, and then wipe it with a dry cloth. Changes or modification not approved by the manufacturer will void the user warranty. Do not disassemble or attempt to repair the device or

components **Calibration and Service**

- · The accuracy of this blood pressure monitor has been carefully tested and is designed for a long service life.
- It is generally recommended to have the device inspected every 2 years to ensure correct functioning and accuracy. Please consult your local OMRON representatives.

5.2 Storage

- Do not store the device in the following situations:
 - · If the device is wet.
 - · Locations exposed to extreme temperatures, humidity, direct sunlight, dust or corrosive vapors such as bleach · Locations exposed to vibrations, shocks or where it will be at an angle
- 6. Specifications

Product category	Electronic Sphygmomanometers
Product description	Upper Arm Blood Pressure Monitor
Model	HEM-7600T
Display	OLED display
Cuff pressure range	Pressure: 0 to 299 mmHg
Measurement range	Pressure: 40 to 260 mmHg
5	Pulse: 40 to 180 beats / min.
Accuracy	Pressure: ±3 mmHg
	Pulse: ±5% of display reading
Inflation	Fuzzy-logic controlled by electric pump
Deflation	Automatic rapid deflation
Measurement method	Oscillometric method
Transmission method	Bluetooth [®] low energy technology
Wireless communication	Frequency range: 2.4 GHz (2400 - 2483.5 MHz)
	Modulation: GFSK
	Effective radiated power: <20 dBm
IP classification	IP 22
Power source	4 "AAA" batteries 1.5V
Battery life	Approximately 300 measurements
Durable merical (Consider life)	(using new alkaline batteries)
Durable period (Service life) Operating conditions	,
Operating conditions	10°C to 40°C / 15 to 90% RH (non-condensing) / 800 to 1060 hPa
Storage / Transport conditions	-20°C to 60°C / 10 to 90% RH (non-condensing)
Weight	Monitor: Approximately 240 g (not including batteries)
Dimensions	Monitor: Approximately 85 mm x 120 mm x 20 mm (not including the arm cuff)
Arm circumference	22 to 42 cm
Contents	Monitor, battery set, instruction manual, setup instructions
Applied part	Type BF
Protection against electric shock	Internally powered ME equipment

Notes:

- · These specifications are subject to change without notice.
- · In the clinical validation study, K5 was used on 85 subjects for determination of diastolic blood pressure
- . This device is clinically investigated according to the requirements of ISO81060-2:2013.
- · This device has not been validated for use on pregnant patients.
- IP classification is degrees of protection provided by enclosures in accordance with IEC 60529. This device is protected against solid foreign objects of 12 mm diameter and greater such as a finger, and against oblique falling water drops which may cause issues during a normal operation.

C€0197

- This device fulfils the provisions of EC directive 93/42/EEC (Medical Device Directive).
- This blood pressure monitor is designed according to the European Standard EN1060, Non-invasive sphygmomanometers Part 1: General Requirements and Part 3: Supplementary requirements for electromechanical blood pressure measuring systems.
- This OMRON product is produced under the strict quality system of OMRON HEALTHCARE Co., Ltd., Japan. The Core component for OMRON blood pressure monitors, which is the Pressure Sensor, is produced in Japan.

Symbol descriptions		
	Please consult this instruction manual	
*	Applied part - Type BF Degree of protection against electric shock (leakage current)	
(((••)))	To indicate generally elevated, potentially hazardous levels of non-ionizing radiation, or to indicate equipment or systems e.g. in the medical electrical area that include RF transmitters or that intentionally apply RF electromagnetic energy for diagnosis or treatment.	
	Temperature limitation	
<u>)</u>	Humidity limitation	
\$••\$	Atmospheric pressure limitation	
ART. or O	Artery mark	

About a wireless communication interference

This Product operates in the unlicensed ISM band at 2.4GHz. In case this Product is used around the other wireless devices including microwave and wireless LAN, which operate same frequency band of this Product, there is a possibility that interference occurs between this Product and such other devices. If such interference occurs, please stop the operation of other devices or relocate this Product before using this Product or do not use this Product around the other wireless devices.

Correct Disposal of This Product

(Waste Electrical & Electronic Equipment) This marking shown on the product or its literature, indicates that it should not be disposed of, with other household wastes at the end of its working life. To prevent possible harm to the environment or human health from uncontrolled waste

disposal, please separate this product from other types of wastes and recycle it responsibly to promote the sustainable reuse of material resources.

Household users should contact either the retailer where they purchased this product, or their local government office, for details of where and how they can return this item for environmentally safe recycling.

Business users should contact their supplier and check the terms and conditions of the purchase contract. This product should not be mixed with other commercial waste for disposal.

7. Tradema	arks	
8 Bluetooth [°]	trademarks owned by Bl such marks by OMRON	ark and logos are registered uetooth SIG, Inc. and any use of HEALTHCARE Co., Ltd. is under ks and trade names are those of
and other countries	e logo are trademarks of s. App Store is a service r e Play logo are trademark	
8. Some U	seful Information	about Blood Pressure
arteries. Arterial blo neart's cycle. The highest pressu owest is the Diasto	ood pressure is constantly re in the cycle is called th blic Blood Pressure. Both	blood flowing against the walls of the y changing during the course of the ne Systolic Blood Pressure; the pressures, the Systolic and o evaluate the status of a patient's
the bio-electrical sy	dition where the heartbea stem that drives the hear , premature contraction, a	at rhythm is abnormal due to flaws in rtbeat. Typical symptoms are an abnormally rapid (tachycardia) or
Why is it a Go Home?	od Thing to measu	re Blood Pressure at
anxiety, or the time your blood pressur measurement may accurate diagnosis Thus it is best to try blood pressure at t	not be sufficient for an	Dyper curve: systolic blood pressure Lower curve: disatolic blood pressure Lower curve: disatolic blood pressure for the system of the system

changes in blood pressure. Blood pressure is typically low in the morning and increases from afternoon to evening. It is lower in the summer and higher in the winter

Manufacturer	OMRON HEALTHCARE Co., Ltd. 53, Kunotsubo, Terado-cho, Muko, KYOTO, 617-0002 JAPAN		
EU-representative	OMRON HEALTHCARE EUROPE B.V. Scorpius 33, 2132 LR Hoofddorp, THE NETHERLANDS		
Asia Pacific HQ	OMRON HEALTHCARE SINGAPORE PTE LTD. 438A Alexandra Road, #05-05/08, Alexandra Technopark, Singapore 119967 www.omronhealthcare-ap.com		
Production facility	OMRON HEALTHCARE Co., Ltd. Matsusaka Factory 1855-370, Kubo-cho, Matsusaka-shi, Mie, 515-8503 Japan		

Made in Japan

